

# BOSTER BIOLOGICAL TECHNOLOGY, LTD.

3942 B Valley Ave, Pleasanton, CA, 94566 Phone: 925-485-4527. 888-466-3604 Fax: 925-485-4560

[www.bosterbio.com](http://www.bosterbio.com)

## Boster Biotech Certificate of Analysis

Note: this is a sample COA. To get the COA for your lot #, please contact us at [support@bosterbio.com](mailto:support@bosterbio.com)

To whom it may concern,


This letter attests that Human THBS1/TSP1/Thrombospondin-1 ELISA Kit ELISA Kit, catalog # EK0899, Lot # (this is SAMPLE COA) is manufactured by Boster Biological Technology, Ltd; through test and assay, we got the following data:

### 1. Typical Data

The following data were obtained for the various standards over the range of 1.56 ng/ml - 100 ng/ml Human THBS1/TSP1/Thrombospondin-1 ELISA Kit , plus the blank well.

Concentration (ng/ml)	0	1.56	3.12	6.25	12.5	25	50	100
O.D.	0.116	0.225	0.297	0.401	0.747	1.194	1.693	2.074

### Standard Curve

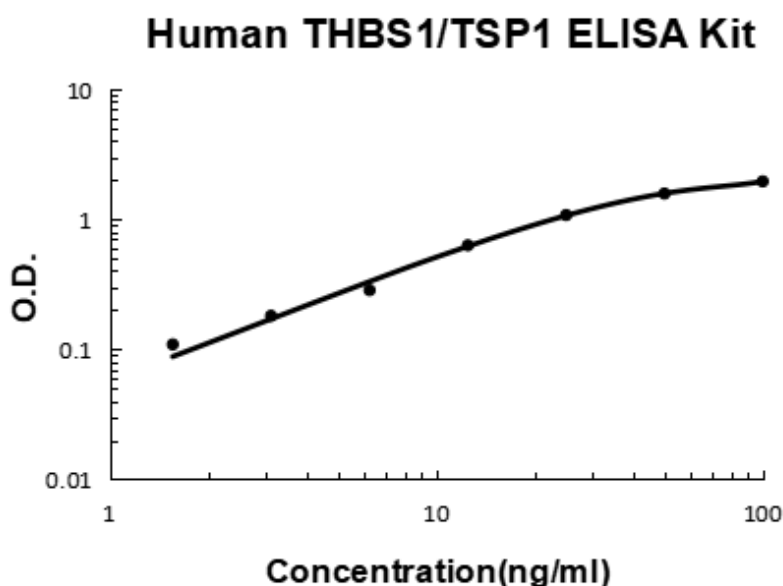

**2. Intra-Assay Precision** Samples of known Human THBS1/TSP1/Thrombospondin-1 ELISA Kit concentration were assayed in replicates of 16 to determine precision within an assay.

The %CV (Coefficient of Variation) of intra-assay is < 10%


3. **Inter-Assay Precision** Samples were assayed 48 times in multiple assays to determine precision between assays.

The %CV (Coefficient of Variation) of inter-assay is < 10%

4. **Sensitivity** The minimum detectable dose of Human THBS1/TSP1/Thrombospondin-1 ELISA Kit is <50 pg/ml. This was determined by adding two standard deviations to the mean O.D. Obtained when the zero standard was assayed 30 times.

5. **Expiration Date** Since the manufacture date for this kit is May 13, 2016, so, it can be stored at 4 degree for 6 months (November 13, 2016), and at -20 degree for 8 months (May 13, 2017). Note: these dates are demo data and not corresponding to the lot you are going to purchase. To get the COA for your particular lot, please contact us at [support@bosterbi.com](mailto:support@bosterbi.com)

Approved by:

A handwritten signature in blue ink, appearing to read '杨静' (Yang Jing), is positioned above the printed name.

Ms. Yangjing Yue Chief technician

Quality Control System of ELISA

Date: May 13, 2016